*Fig. 1*

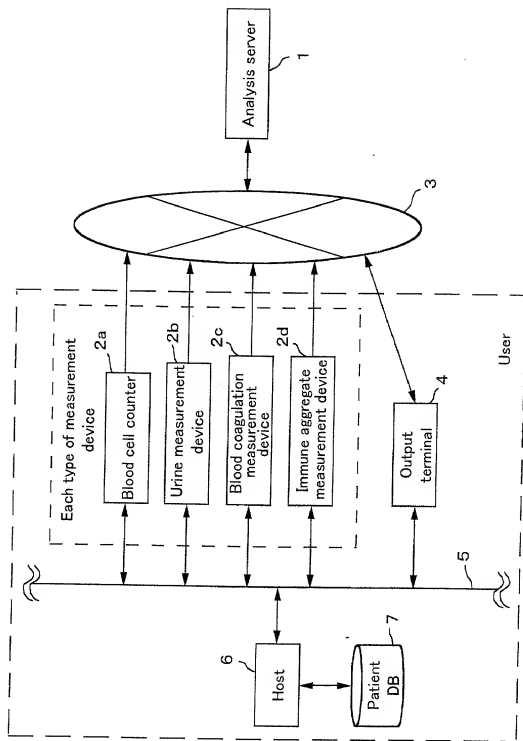


Fig. 2

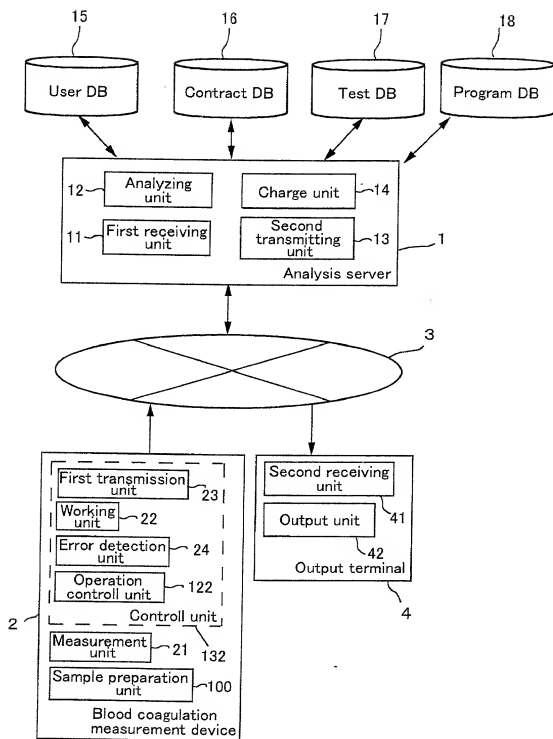


Fig. 3

User ID	U—sysmex	
User Name	Sysmex Hospital	
Contact Person	Test Dept.: Tanaka	
Contract details	123-4567	
Actual Usage	Analysis service ID	Number of times of use
	BASIC	100
	COO1	60
	COO2	37

Fig. 4

102280-1251260

Contract details	Analysis service ID	Test items	Basic contract flag	Basic unit cost	Max. number of uses
123-4567	BASIC	APTT, PT, Fbg	Yes	¥15,000	100
123-4567	C001	APTT, PT, Fbg	No	¥200	—
123-4567	C002	TTO	No	¥450	—

Fig. 5

User ID	U—sysmex
Specimen ID	01-001
Device ID	M103
Analysis order	6789
Sample classification	Blood
Test item	PT
Measurement item	PT
Device class	Sysmex CA-1500 α
Device version	Ver. 03
Reply address	out@U—sysmex. co. jp
Correction value	1
Measurement data	(2,28)、(2.1,31)、(2.2,35)……

Fig. 6A

Measurement data	Intensity of the scattered light (%)
2	28
2.1	31
2.2	35
10.9	49
11	50
11.1	52
22	100

Fig. 6B

User ID	U—sysmex
Specimen ID	01-001
Device ID	M103
Analysis order	6789
Sample class	Blood
Test item	PT
Device class	Sysmex CA-1500
Analysis data	11.0sec.
Supplemental info.	110.5% 1.04 1.07INR

Fig. 7

10220-121600

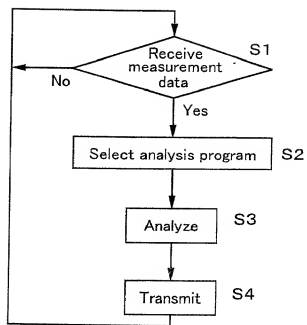
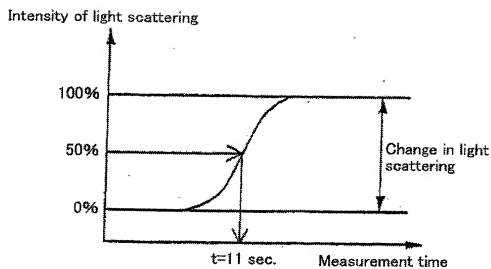


Fig. 8

*Fig. 9*

00034521-002701

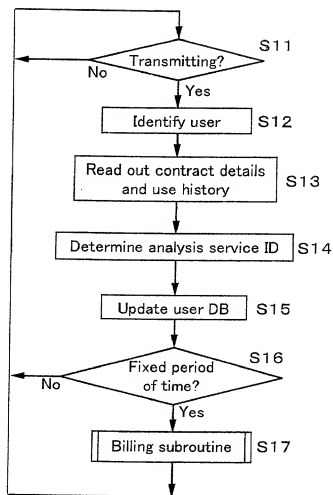


Fig. 10

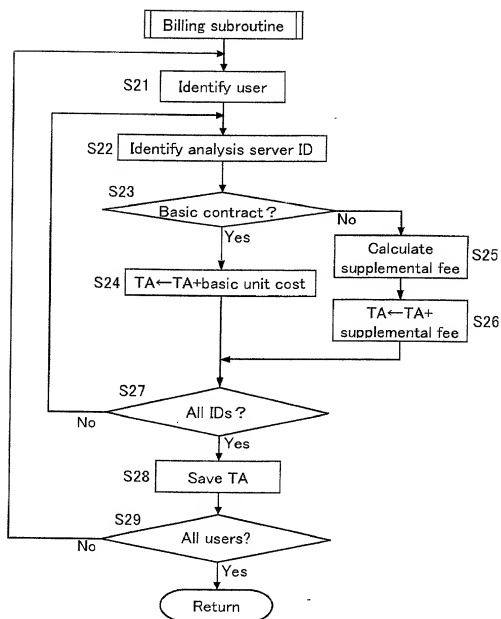


Fig. 11

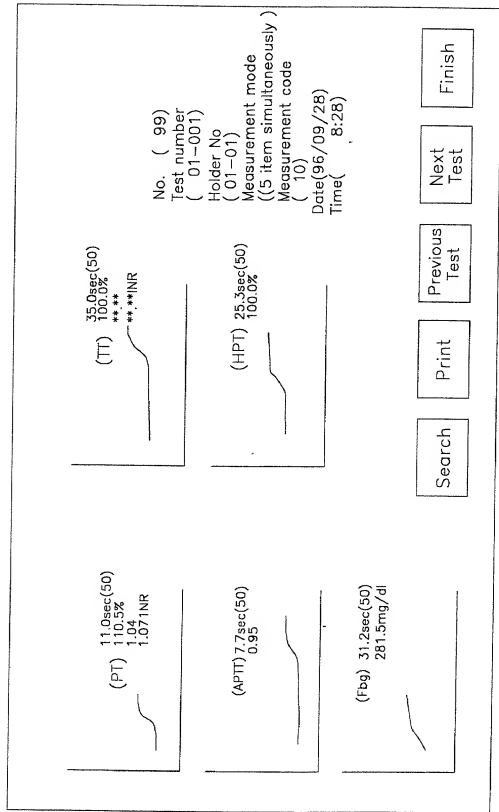


Fig. 12

00034521-000301

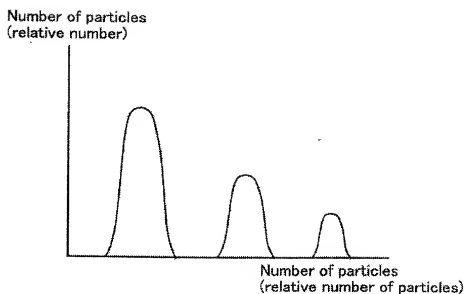


Fig. 14

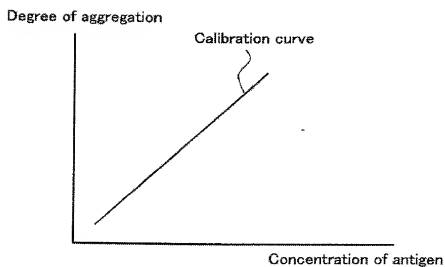


Fig. 15

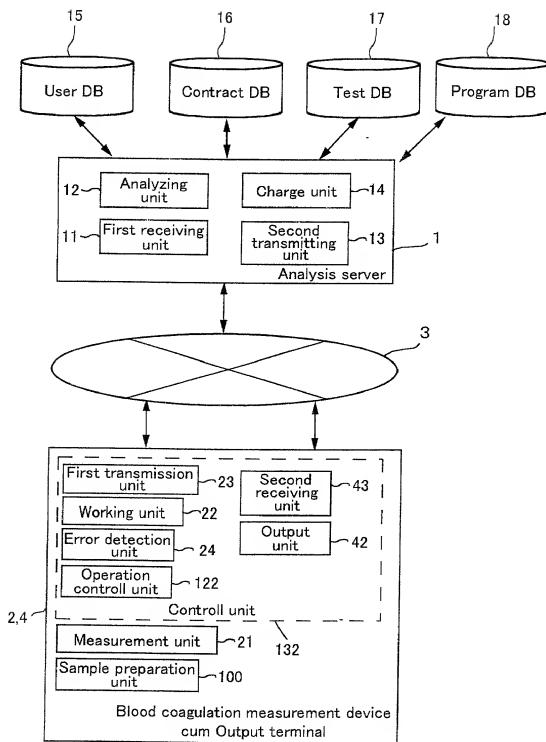


Fig. 16

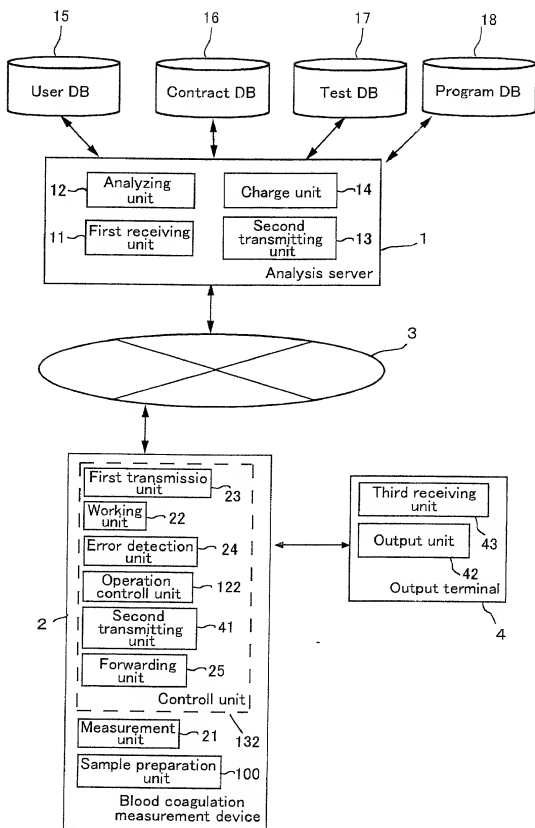


Fig. 17

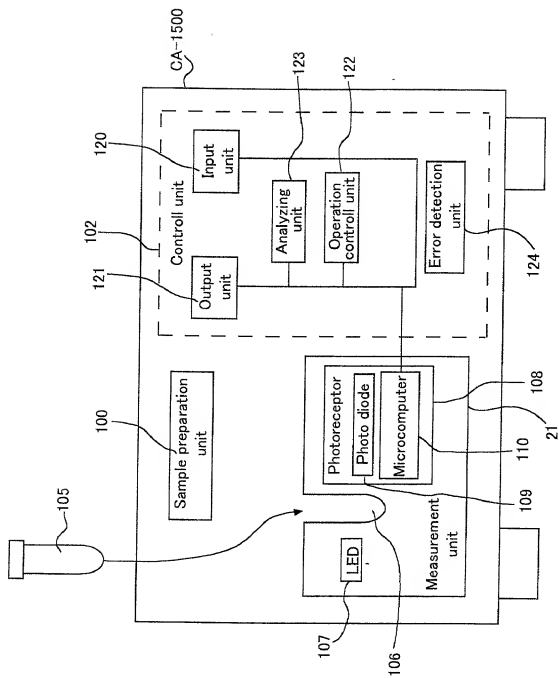


Fig. 18

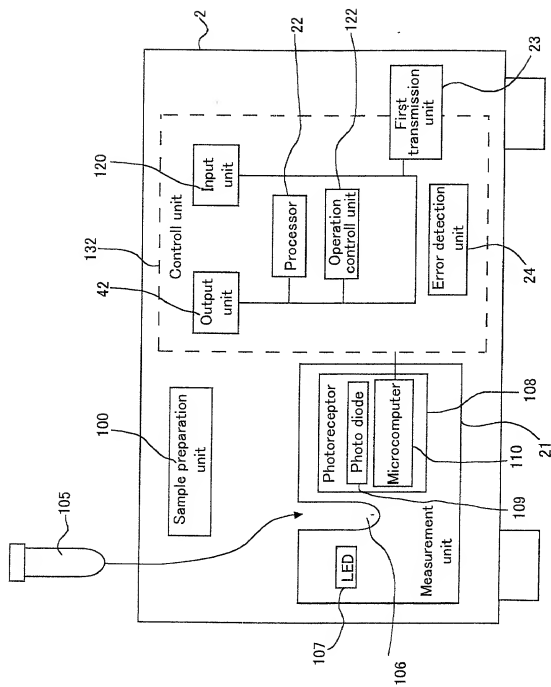


Fig. 19